

#4

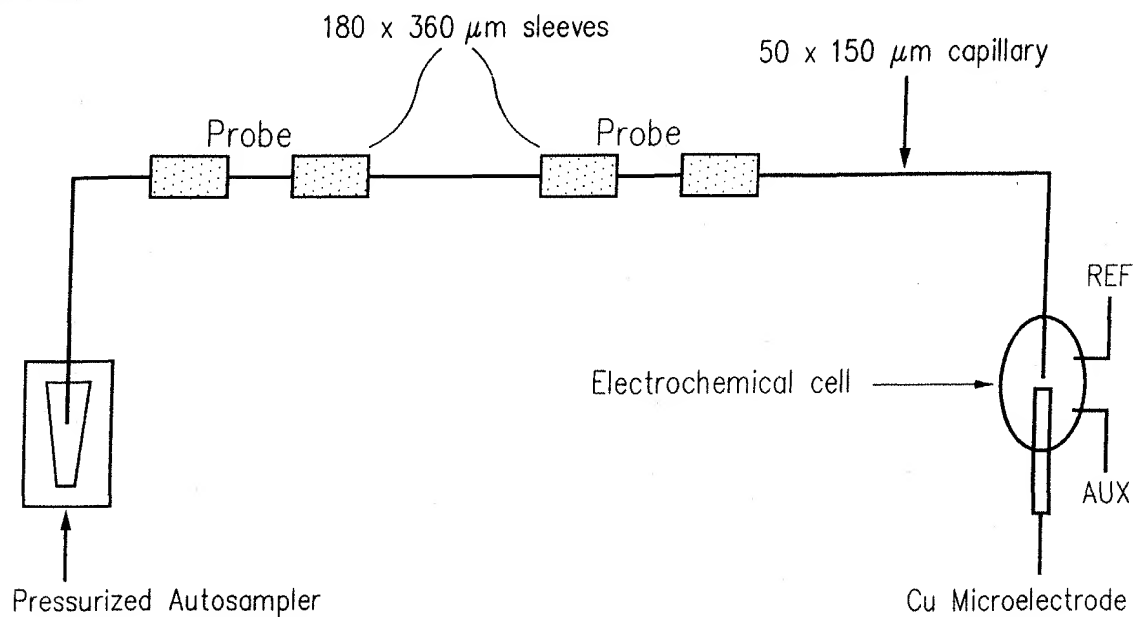


FIG. 1

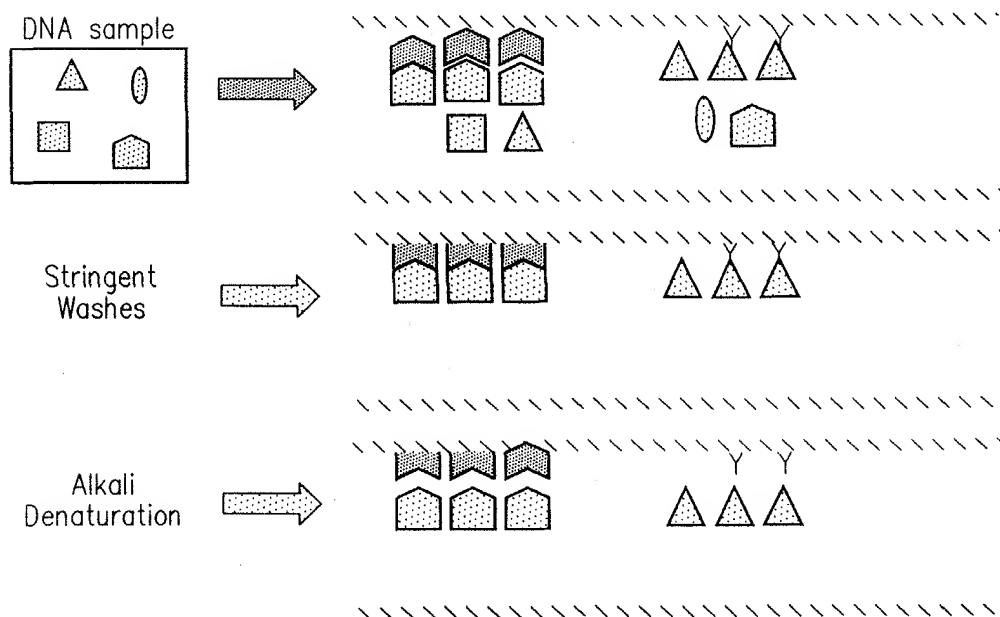


FIG. 2

09874400-011502


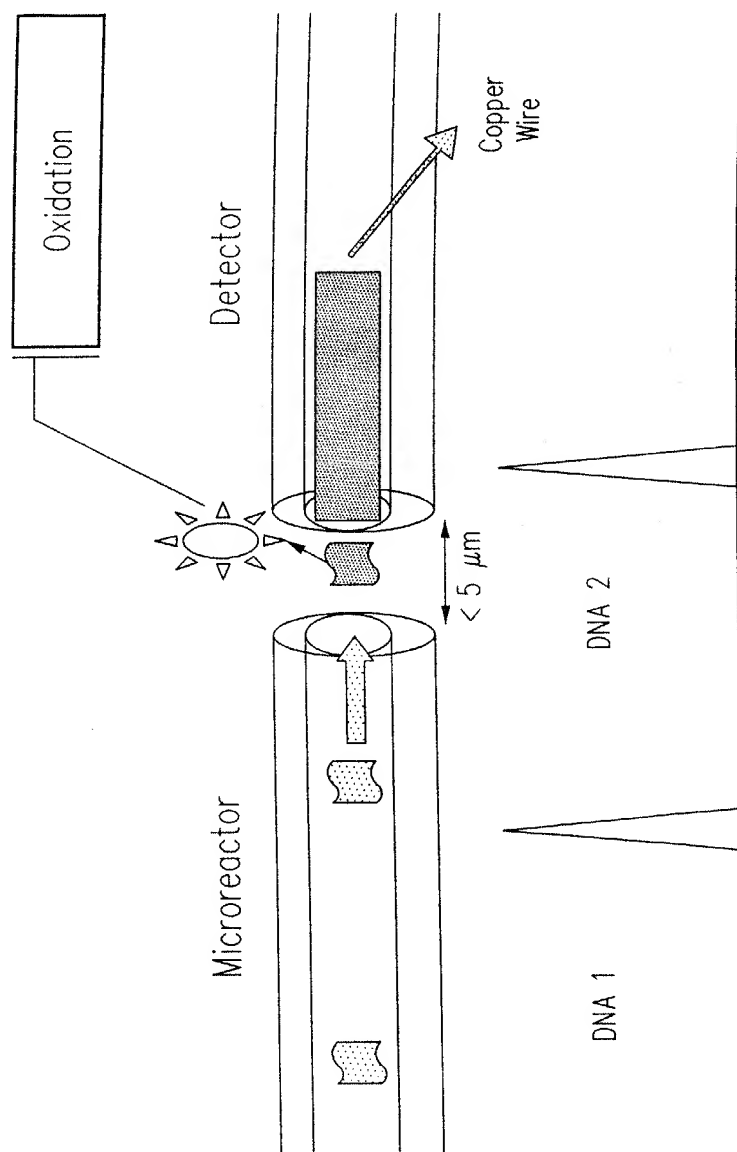


FIG. 3

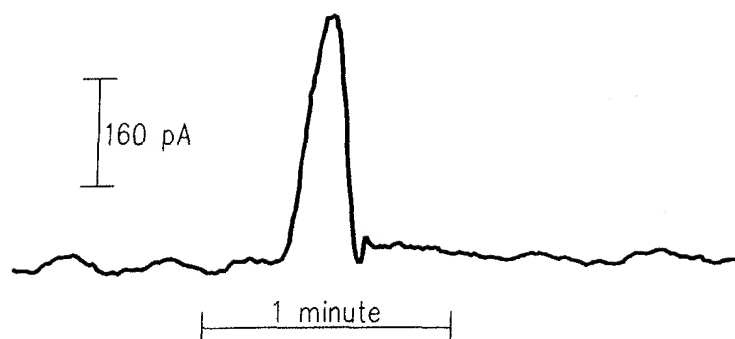

Capillary DNA-biosensor with TB+HIV Probes Immobilized.  
 Length of each probe zone = 1 cm. Distance between zones = 7 inches  
 Elution of Target with TBE buffer, pH = 11, after 30 minute incubation  
 Detection: Sinusoidal voltammetry with  $40\text{ }\mu\text{m}$  Copper electrode  
 2 Hz, 0-700 mVp-p sine wave. Response shown at 5th Harmonic.

FIG. 4

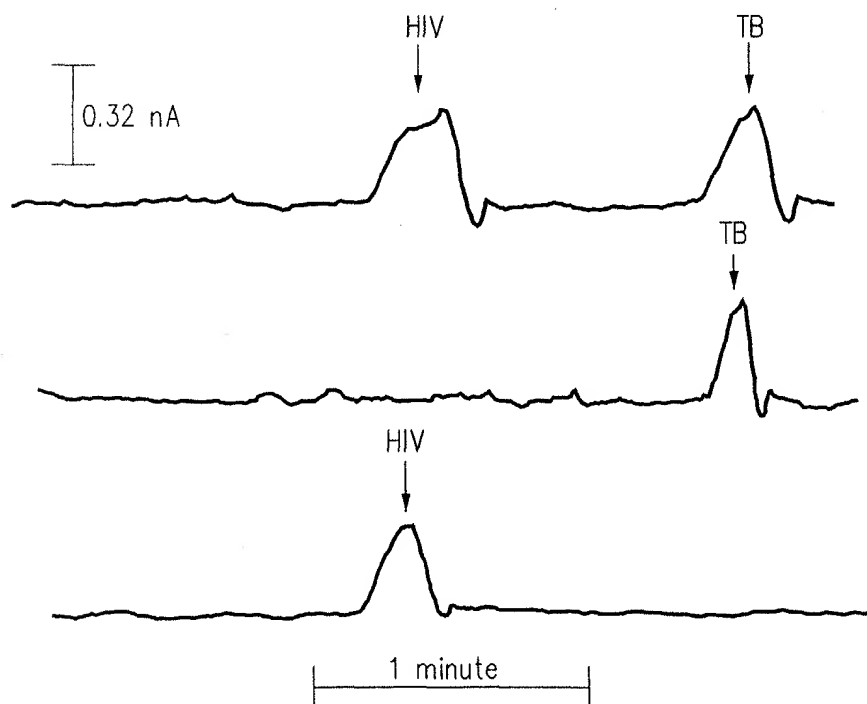


FIG. 5

20570-00442860

205710-0044/860

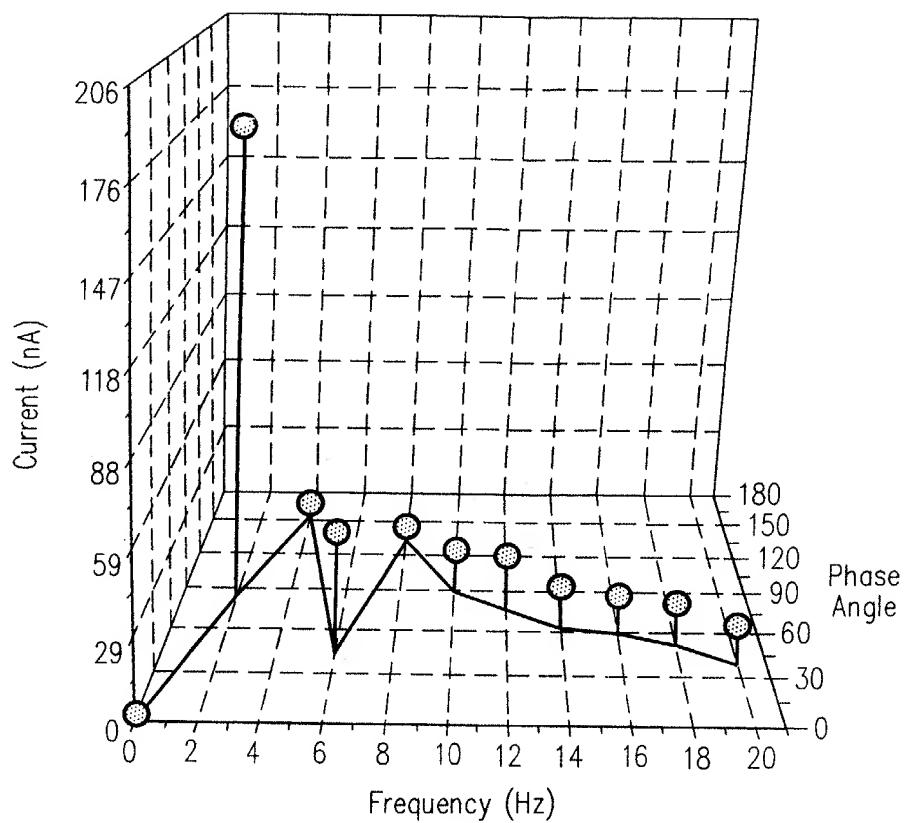


FIG. 6

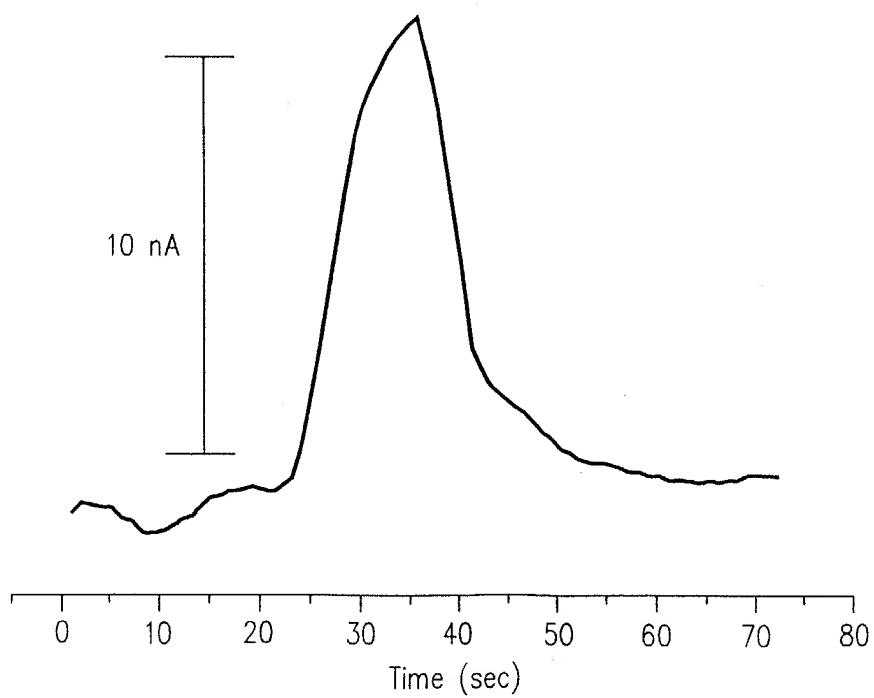


FIG. 7

205110-0044/860

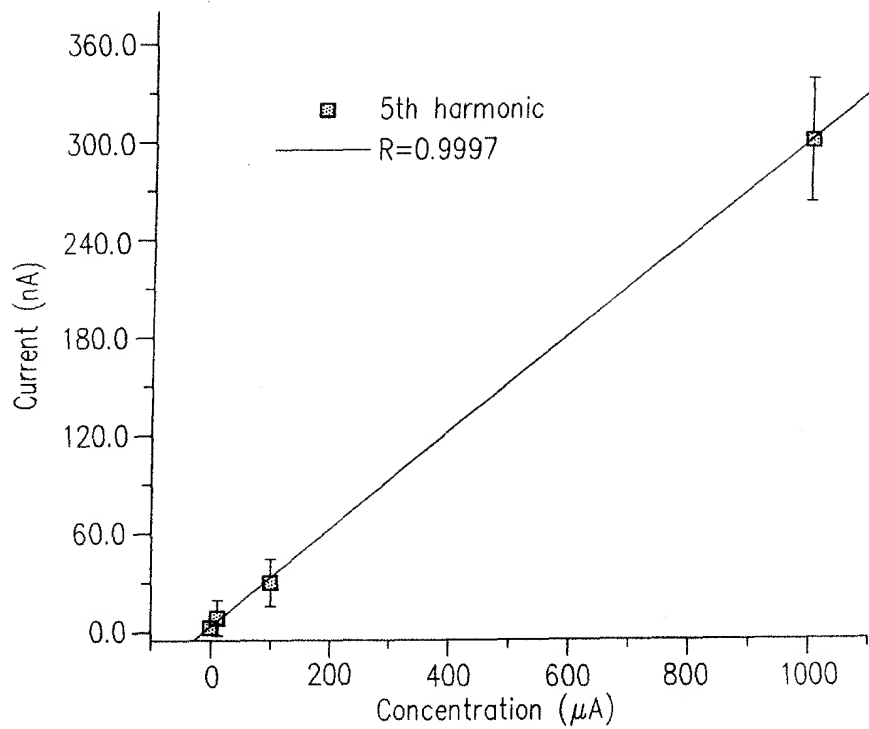


FIG. 8

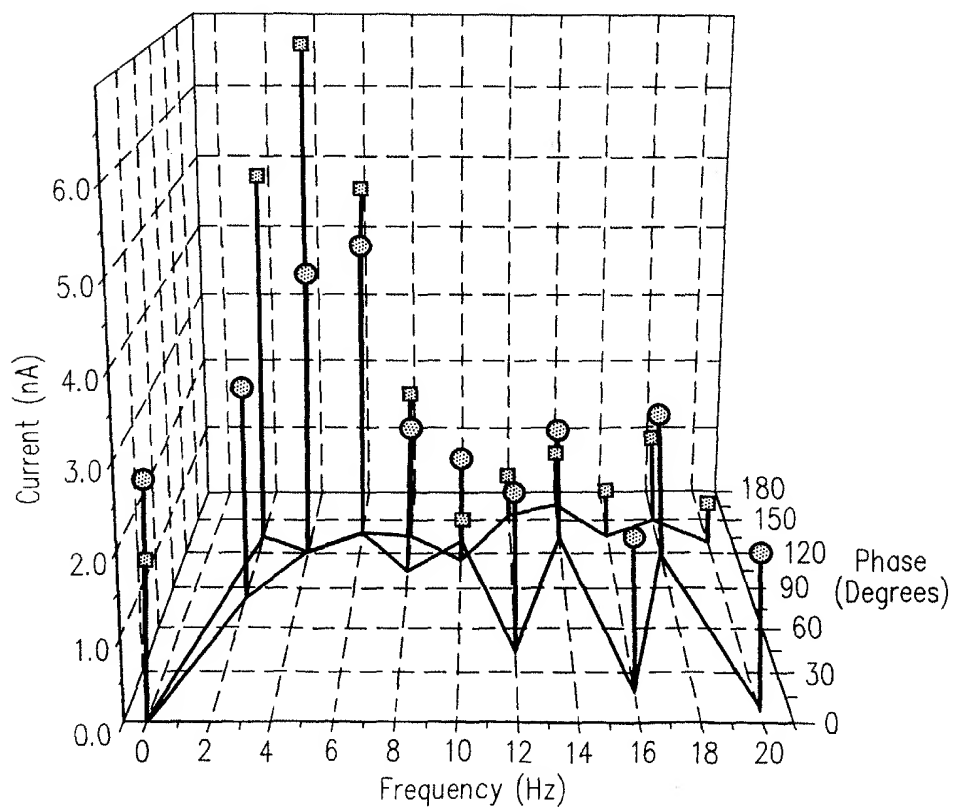


FIG. 9

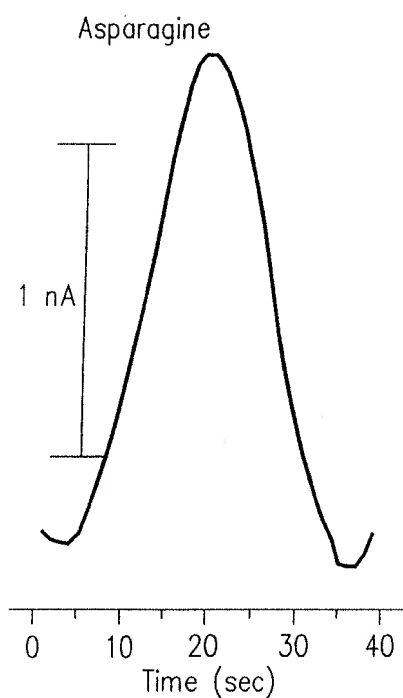


FIG. 10A

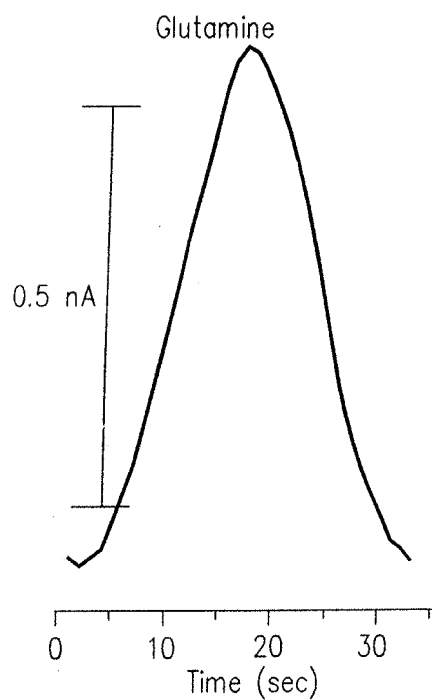


FIG. 10B

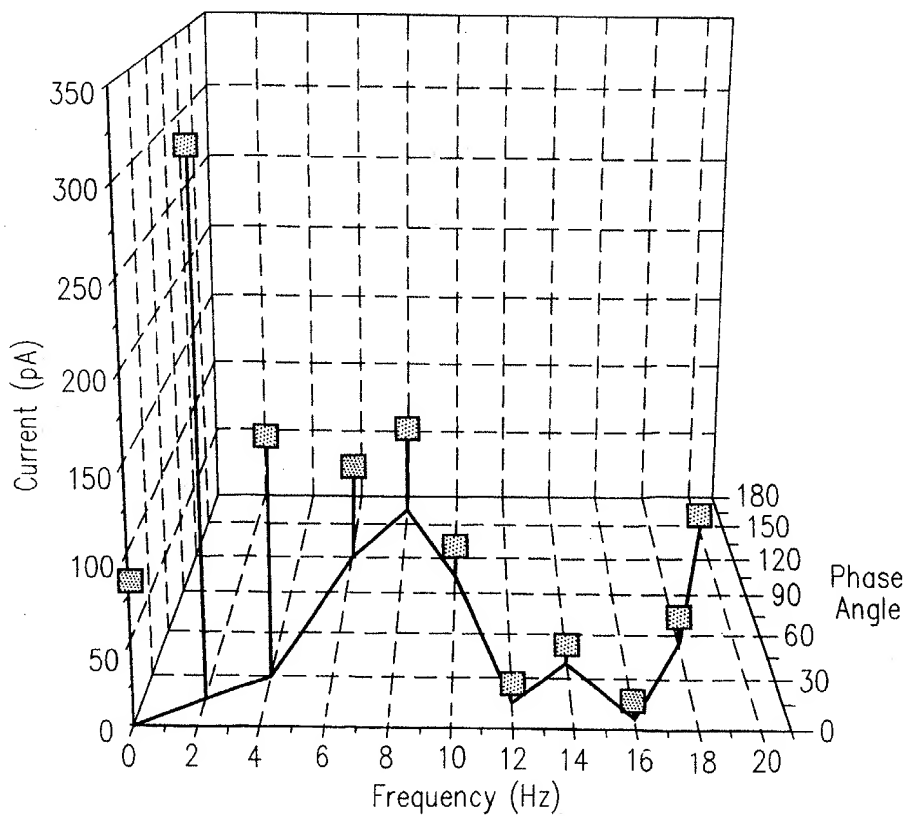


FIG. 11

205110-0044260

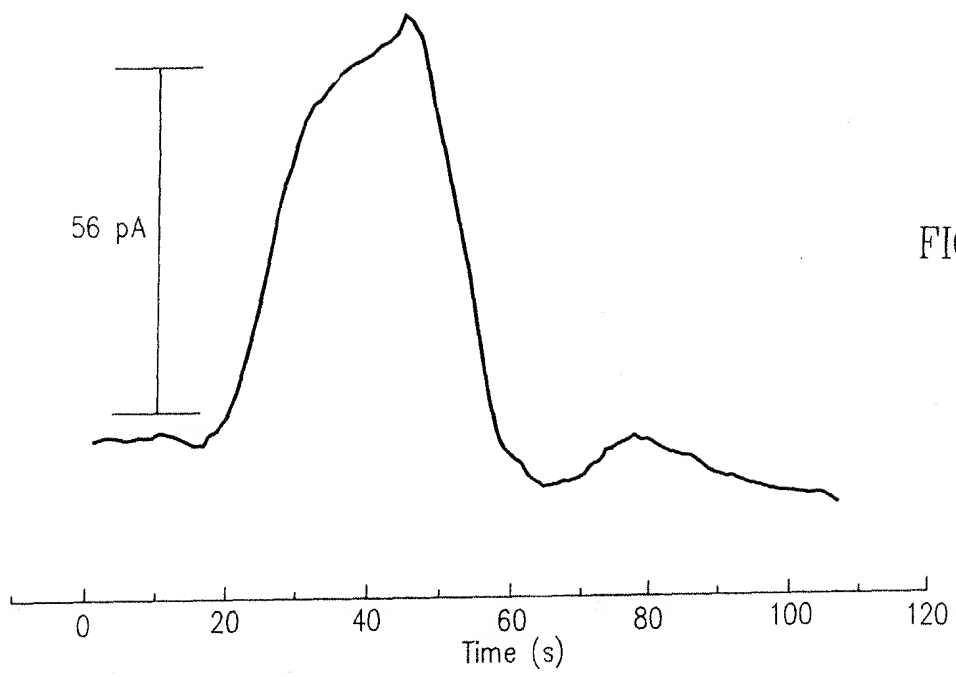


FIG. 12




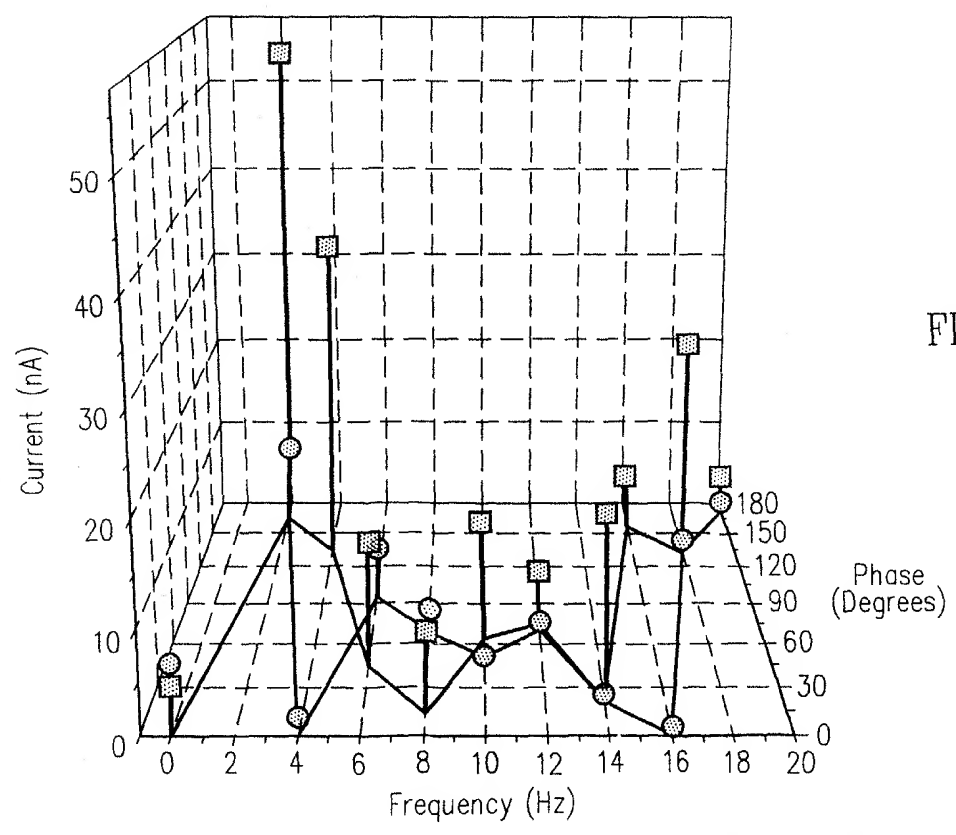


FIG. 13

205110-0047/860

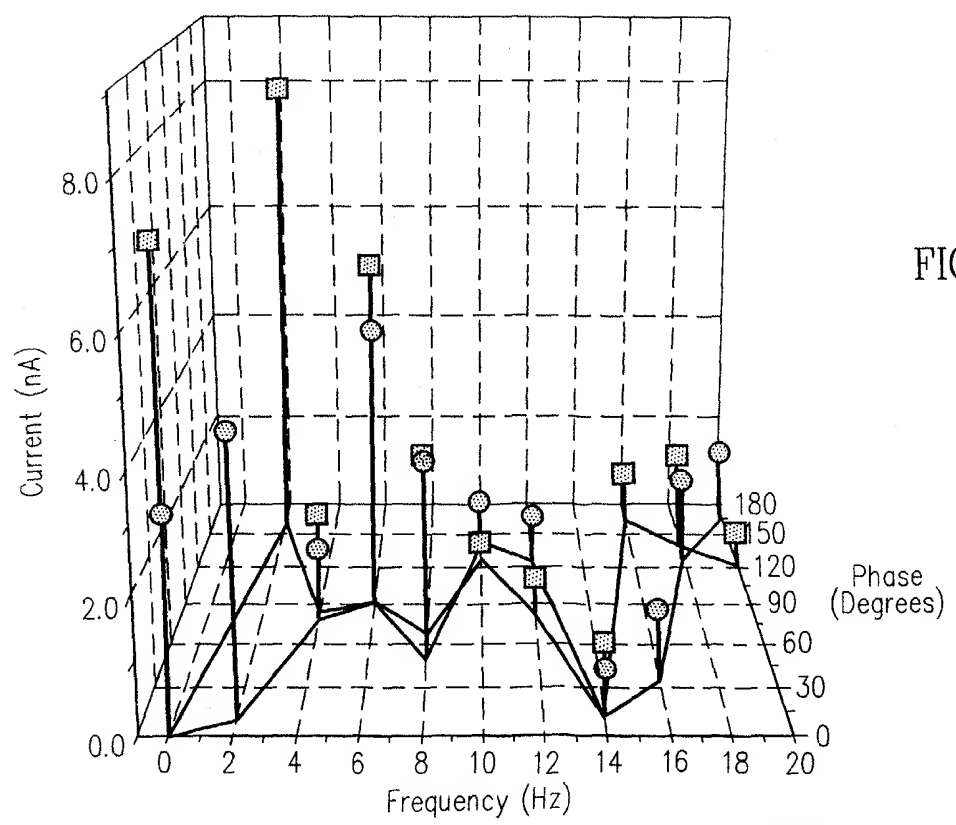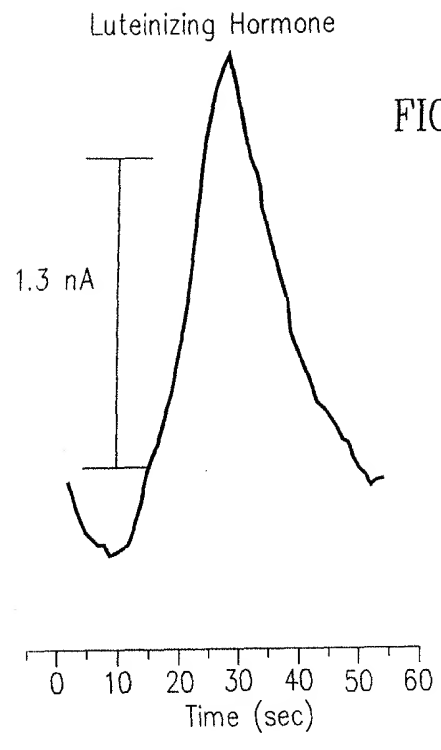

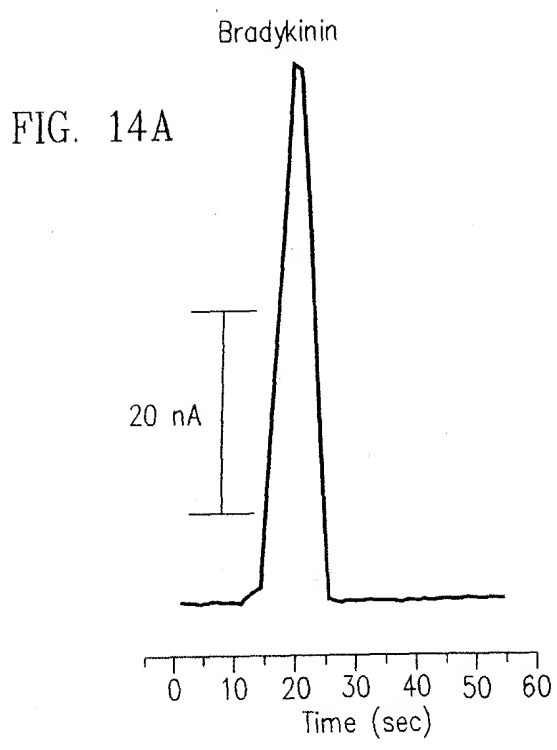

09274400.01500

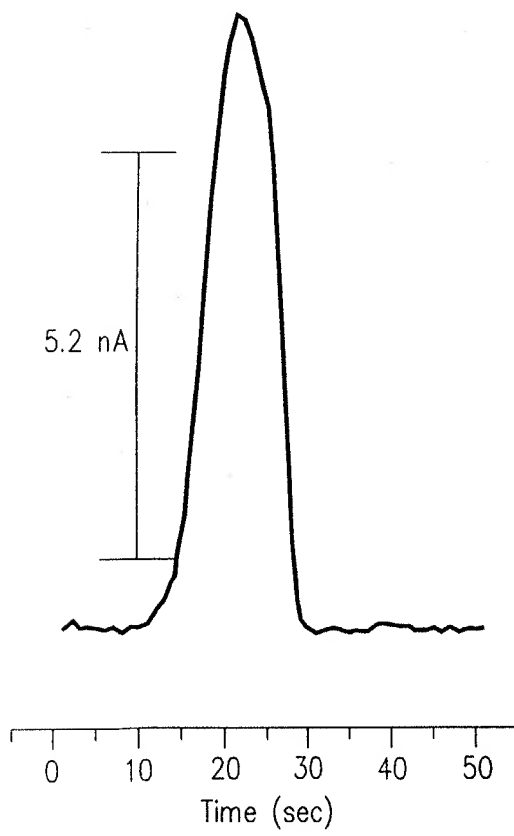


FIG. 16A

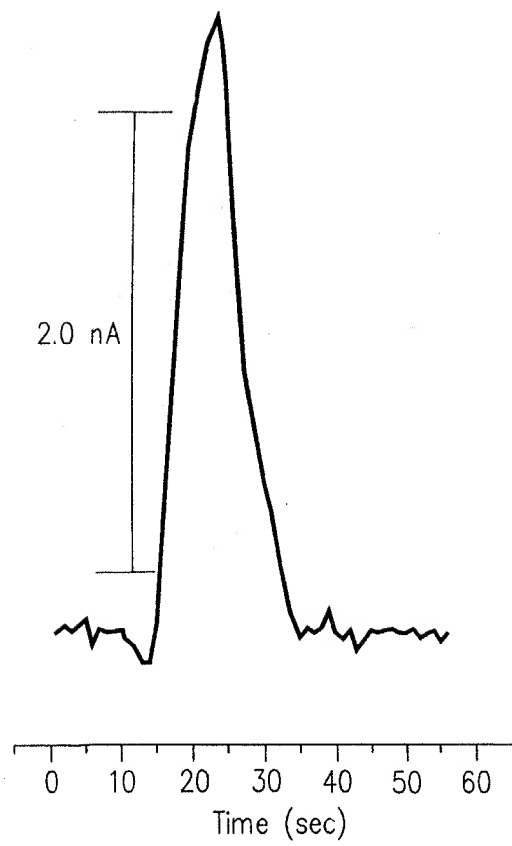


FIG. 16B